

**NOTES :**

**GENERAL**

OUTPUT TO THE INSTRUMENT FROM THE PREAMP IS A GAIN OF 1.


WHEN A COMBINATION ELECTRODE IS USED, REFERENCE CONNECTION IS MADE THROUGH THE BNC CONNECTOR. USE OF A SEPARATE REFERENCE REQUIRES THAT ITS LEAD BE CONNECTED DIRECTLY TO THE Iso Grd TERMINAL IN THE INSTRUMENT.

**TEMPERATURE COMPENSATION**


STANDARD AUTO TC IS ACCOMPLISHED WITH A 3KΩ BALCO ELEMENT ACROSS T+ AND T-.

**SHIELDING**

TAKE CARE NOT TO ALLOW THE BNC SHIELD (REFERENCE LEAD) TO CONTACT METAL PIPING OR J-BOXES AT ANY POINT, AS THIS WILL SHORT THE REFERENCE CELL TO EARTH GROUND, AND CAUSE UNSTABLE READINGS. SHIELDING OF THE CABLE FROM AMPLIFIER TO INSTRUMENT IS USUALLY NOT REQUIRED. IF A SHIELD IS USED, CONNECT IT TO THE **SENSR GND** TERMINAL #13, AND MAKE SURE THAT IT DOES NOT TOUCH ANY OF THE OTHER LEADS, OR EARTH GROUND.

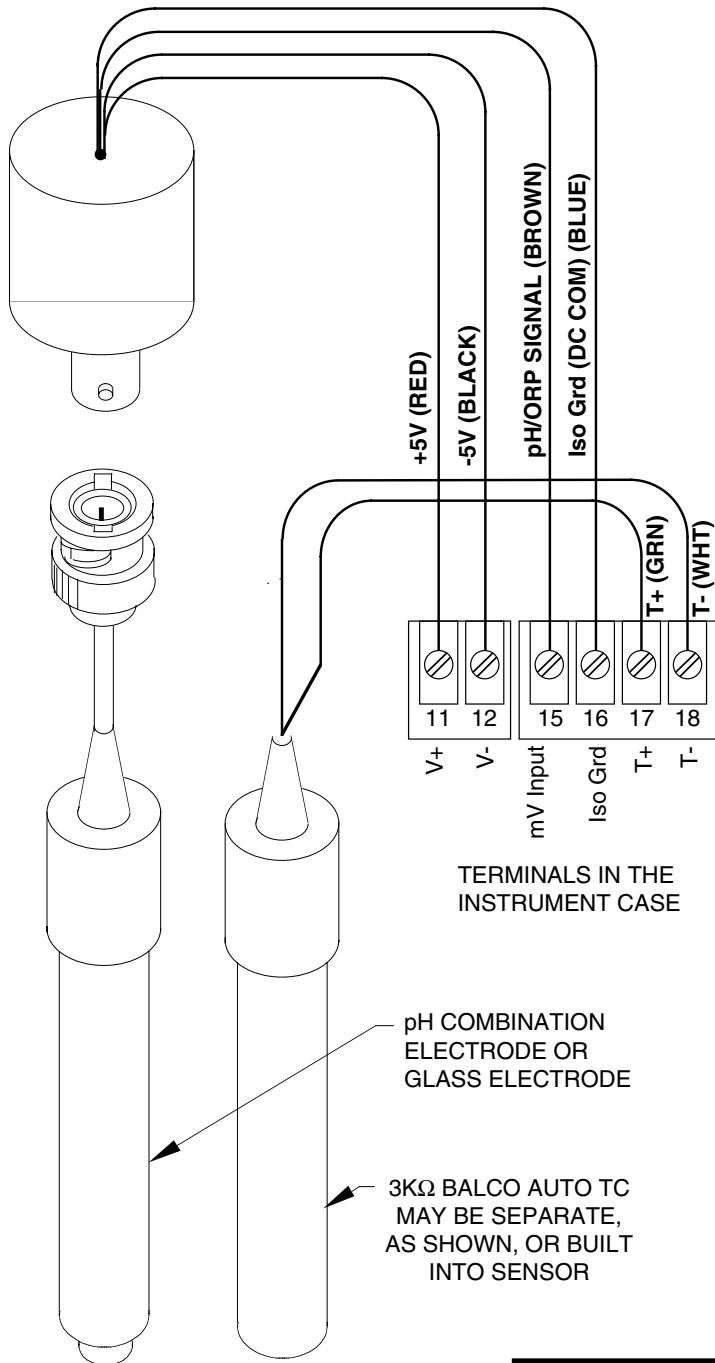

NOTES UNLESS OTHERWISE SPECIFIED:

		11751 Markon Drive	
		Garden Grove, CA. 92841 USA	
		phone: 714-895-4344 fax: 714-894-4839	
DRAWN 6/19/02rh	TITLE		
CHECKED	<b>SSA2 WITH SIGNET 8750-2</b>		
APPROVED	SCALE NONE	DRAWING NO.	REV.
	SHEET 1 OF 1	<b>SSA2-8750-2</b>	